

IN THE UNITED STATES PATENT AND TRADEMARK OFFICE

In re US Patent Application of

Shiro.KANEGASAKI

Serial No. : 10/542,189

Filing date : April 8, 2004

For : APPARATUS FOR DETECTING CHEMOTAXIS OF CELLS

VERIFICATION OF TRANSLATION

Honorable Commissioner of Patents and Trademarks

Washington, D.C. 20231

Sir :

I, Katsufumi HIRATA, residing at 20-25, Nishishinagawa 3-chome, Shinagawa-ku, Tokyo, Japan, declare and state :

- (1) that I am able to read and understand well both the Japanese and English languages;
- (2) that I supervised the translation of the Japanese Patent Application No. 105197/2003 from Japanese to English;
- (3) that the attached English translation is a true and correct translation of the above-identified Application to the best of my knowledge and belief; and
- (4) that all statements made of my own knowledge are true and that all statements made on information and belief are believed to be true, and further that these statements are made with the knowledge that willful false statements and the like are punishable by fine or imprisonment, or both, under 18 USC 1001, and that such false statements may jeopardize the validity of the application or any patent issuing thereon.

Date : May 10, 2006

Katsufumi Hirata
Signature: Katsufumi HIRATA

【Name of Document】 Request for Patent

【Serial No.】 SP0062SSK

【Filing Date】 April 9, 2003 (Heisei 15)

【Address】 Commissioner of the Patent Office

【Int. Cl.】 C12M 1/32

【Inventor】

【Domicile or Residence】 21-2-503, Masukata 1-chome, Tama-ku,
Kawasaki-shi, Kanagawa

【Name】 Shiro KANEGASAKI

【Applicant】

【Identification No.】 500201406

【Name】 Effector Cell Institute, Inc.

【Representative】

【Identification No.】 100082739

【Patent Attorney】

【Name】 Katsuo NARUSE

【Nominated Representative】

【Identification No.】 100083080

【Patent Attorney】

【Name】 Katsufumi HIRATA

【Indication of Fee】

【Deposit Account No.】 011970

【Amount of Payment】 21,000 Yen

【List of Submitted Documents】

【Article】 Specification 1

【Article】 Drawings 1

【Article】 Abstract 1

【Number of General Power of Attorney】 0202868

【Proof of Receipt】 Requested

【Name of Document】 SPECIFICATION

【Title of the Invention】

APPARATUS FOR DETECTING CHEMOTAXIS OF CELLS

【Claims】

【Claim 1】 An apparatus for detecting chemotaxis of cells with a structure wherein plural number of wells are connected to each other via a channel and each well has an opening for injecting cells or a specimen, characterized by having a means of sealing the all opening(s) in one or both of the cell-injection side and the specimen-injection side.

【Claim 2】 The apparatus for detecting chemotaxis of cells as claimed in claim 1 characterized in that said channel has resistance to fluids of suspended cells.

【Claim 3】 The apparatus for detecting chemotaxis of cells as claimed in claim 1 or 2 characterized by having a means of transporting a liquid in order to transfer the cells.

【Claim 4】 The apparatus for detecting chemotaxis of cells as claimed in claim 3 characterized in that said means of transporting a liquid has a means of stopping the transportation of the liquid after injecting or aspirating/discharging thereof.

【Claim 5】 The apparatus for detecting chemotaxis of cells as claimed in claim 2 comprising a substrate having plural number of wells provided in both sides of a bank and a glass substrate pressed against the substrate, wherein said channel formed

between the bank and the glass substrate has resistance to the passage of suspended cells.

【Claim 6】 The apparatus for detecting chemotaxis of cells as claimed in claim 5 characterized in that said substrate or a gap between said substrate and said glass substrate has an opening in order to transport a liquid.

【Claim 7】 The apparatus for detecting chemotaxis of cells as claimed in claim 5 characterized in that one of said wells provided in said substrate has an opening for injecting cells and the other well has an opening for injecting specimen.

【Claim 8】 The apparatus for detecting chemotaxis of cells as claimed in claim 7 characterized in that the means of sealing said opening(s) in one or both of the cell-injection side and the specimen-injection side is a member selected from among a flexible stopper, a slide-type switching member, a tap, a valve and a combination thereof.

【Claim 9】 The apparatus for detecting chemotaxis of cells as claimed in claim 5 characterized in that a terrace is formed on the upper part of said bank in the channel and a gap fit for the diameter or deformability of cells is formed between said terrace and said glass substrate.

【Claim 10】 The apparatus for detecting chemotaxis of cells as claimed in claim 9 characterized in that on said terrace on the upper part of said bank in said channel, barriers constituting one or more grooves having a width and/or a depth

fit for the diameter or deformability of cells are provided, and if desired, a gap fit for the diameter or deformability of cells between said barriers and said glass substrate is also formed.

[Claim 11] The apparatus for detecting chemotaxis of cells as claimed in claim 10 characterized in that in said channel, arrays of barriers constituting one or more grooves are formed at two positions of said terrace.

[Claim 12] The apparatus for detecting chemotaxis of cells as claimed in claim 9 characterized in that a multistage bank is formed in said channel in order to form gaps having different depth between said terrace and said glass substrate.

[Claim 13] An integrated apparatus for detecting chemotaxis of cells characterized in that said apparatuses as claimed in claims 1 to 12 are each referred to as a single unit and the plural number of units of one or more types are integrated.

[Claim 14] The integrated apparatus for detecting chemotaxis of cells characterized in that said integrated apparatuses as claimed in claim 13 are each referred to as a single unit and the plural number of units of one or more types are integrated.

[Detailed Description of the Invention]

[0001]

[Technical Field to which the Invention Pertains]

This invention relates to an apparatus for detecting chemotaxis of cells.

【0002】

More particularly, it relates to an apparatus by which chemotaxis of cells can be detected by using a microquantity of cells and which has a structure ensuring to easily control cell positioning in a microwell and maintain a stable concentration gradient of a specimen such as a chemotactic factor in a channel.

【0003】

【Prior Arts・Problems to be solved by the Invention】

As will be discussed hereinafter, the present inventors have made several proposals about apparatuses for detecting chemotaxis of cells by which chemotaxis of cells can be detected with the use of a microquantity of cells by supplying a cell suspension into a well, supplying a specimen into another well and examining whether or not the cells migrate toward the well containing the specimen via a channel provided between the wells. Use of an apparatus for detecting chemotaxis of cells enabling the observation and detection at the single cell level and allowing measurement with the use of about 100 cells, if possible, offers such advantages that scarce cells can be easily examined and cell reactions can be quantitatively studied. In a structure wherein individual wells, which are connected to each other via channels, have each a cell injection port and a specimen injection port, wells together form a connecting tube via the channels and, in its turn, a liquid frequently migrates

in the channels. In the step of injecting a specimen such as cells into a well, namely, there frequently arises an increase in pressure, which results in unexpected migration of cells or the specimen in many cases. In the case wherein wells are not completely leveled after the injection or micromovements occur on the liquid level due to, for example, vibration, the transportation of the liquid in the channel is amplified so as to frequently cause migration of cells or a specimen. Such unexpected migration of cells or a specimen causes confusion in the judgment whether the specimen is a chemotactic factor or not. To accurately detect the migration of cells, which perceive the concentration gradient due to the diffusion of the specimen, toward a well containing a specimen, it is therefore required to strictly prevent the unexpected migration of the liquid in the wells involving the channels.

【0004】

The present inventors have previously proposed that, in the case of injecting or aspirating a sample into a well having a tube for injecting/aspirating a sample such as a cell or a chemotactic factor with a micropipette or the like, a rapid change in pressure in a well can be relieved and unexpected migration of the sample in the well can be prevented by providing another tube connecting to the tube for injecting or aspirating the sample (JP-A-2002-159287). In this case, use is made of the structure wherein the pressure in injecting or aspirating

a sample is dispersed through the connecting tube.

【0005】

The present inventors have further proposed a microsample treatment apparatus such as an apparatus for detecting chemotaxis of cells wherein, in a structure comprising a plural number of wells being connected to each other via a part having resistance to fluids and individual wells being provided with tubes for injecting/aspirating a sample and, if necessary, tubes for relieving pressure changes at the injection/aspiration, these tubes have a space in common at the top ends thereof in which a liquid can be held (WO 02/46356). By employing the structure wherein all of the tubes provided in individual wells have a space in common at the top ends thereof in which a liquid can be held, the migration of a liquid at the step of injecting a sample and thereafter can be prevented. In this apparatus, moreover, the positions of the injected cells in a well can be controlled so as to align the cells along the start line at one end of a channel. For this purpose, this apparatus has a means of precisely controlling the injection/discharge of a liquid in a well.

【0006】

To align cells injected into a well along the start line at one end of a channel, the liquid in the well should be moved and delicate control is required therefor. To prevent the subsequent migration of the liquid in the channel, it is also

required to return the liquid into the space at the top ends of the tubes. That is, complicated and strictly controlled procedures are necessary therefor.

【0007】

An object of the present invention is to further improve such an apparatus and thus provide a structure for detecting chemotaxis of cells at an elevated accuracy with the use of a microquantity of cells. Namely, an object of the present invention is to provide an apparatus for detecting chemotaxis of cells by which cells or a specimen can be easily injected and position control of the injected cells can be easily carried out while ensuring the prevention of unexpected migration of the cells definitely positioned in a well or the injected specimen so that a stable concentration gradient due to the diffusion of the specimen can be maintained and which ensures further automated operation and controlling.

【0008】

【Patent Document 1】 JP-A-2002-159287

【Patent Document 2】 WO 02/46356

【Means for Solving Problem】

【0009】

The present invention relates to an apparatus for detecting chemotaxis of cells with a structure wherein plural number of wells are connected to each other via a channel and each well has an opening for injecting cells or a specimen, characterized

by having a means of sealing the all opening(s) in one or both of the cell-injection side and the specimen-injection side and said channel may have resistance to fluids of suspended cells, further in order to transfer the cells, the apparatus may have a means of transporting a liquid, wherein said means of transporting a liquid may have a means of stopping the transportation of the liquid after injecting or aspirating/discharging thereof.

【0010】

The present invention relates to an apparatus for detecting chemotaxis of cells comprising a substrate having plural number of wells provided in both sides of a bank and a glass substrate pressed against the substrate, wherein said channel formed between the bank and the glass substrate has resistance to the passage of suspended cells. And said substrate or a gap between said substrate and said glass substrate may have an opening in order to transport a liquid. Further one of said wells provided in said substrate has an opening for injecting cells and the other well has an opening for injecting specimen and the means of sealing said opening(s) in one or both of the cell-injection side and the specimen-injection side is can be selected from among a flexible stopper, a slide-type switching member, a tap, a valve and a combination thereof.

【0011】

In another embodiment, it is preferable that a gap between the

bank and the glass substrate which has resistance to the passage of suspended cells is formed, and a terrace is provided on the upper part of the bank in said channel and said terrace and said glass substrate forms a gap fit for the diameter or deformability of cells

【0012】

Further it is preferable that on said terrace on the upper part of said bank in said channel, barriers constituting one or more grooves having a width and/or a depth fit for the diameter or deformability of cells are provided, and if desired, a gap fit for the diameter or deformability of cells between said barriers and said glass substrate is also formed. Further in said channel, arrays of barriers constituting one or more grooves may be formed at two positions of said terrace and a multistage bank may be formed in said channel in order to form gaps having different depth between said terrace and said glass substrate.

【0013】

The present invention includes in its scope an integration apparatus for detecting chemotaxis of cells consisting of a plural number of units of the same or different types with the use of the above-described apparatus for detecting chemotaxis of cells as a single unit. Moreover, it includes an integration apparatus for detecting chemotaxis of cells consisting of a plural number of integration units of the same or different types with the use of the above-described integration unit as

a single unit.

【0014】

【Mode for carrying out the Invention】

The apparatus for detecting chemotaxis of cells according to the present invention is an apparatus having a structure wherein plural wells are connected to each other via a channel having resistance to the passage of cells. After supplying a cell suspension in one of these wells, the cells are aligned at one end of the channel. Next, a specimen is supplied into the other well. Thus the passage of the cells perceiving the concentration gradient of the specimen toward the well holding the specimen can be observed or the cells under passage or having been passed can be counted.

【0015】

The channel having resistance to the passage of cells as described above means a flow path for cells having a gap through which a cell in the non-adsorbed state (usually having a spherical shape) cannot pass but a cell changing into a flat shape due to its deformability can pass. The term "deformability" of a cell as used herein means that, in case of a flexible cell, the cell can easily change its shape (for example, into flat or string-shaped cells) owing to the flexibility and thus can pass through a gap having a smaller size than the diameter of the cell being in the inherent spherical shape in a free space.

【0016】

The characteristic of the apparatus for detecting chemotaxis of cells according to the present invention resides in, in addition to the fundamental structure as discussed above, having a means of sealing the opening(s) in one or both of the cell-injection side and the specimen-injection side after the injection of cells into the well. The apparatus for detecting chemotaxis of cells according to the present invention may have a means of transporting cells by injecting or aspirating/discharging a liquid and said means of injecting or aspirating/discharging a liquid may have a means of stopping the transportation of the liquid after the injection or aspiration/discharge in order to enable seal the opening(s) in one or both of the cell-injection side and the specimen-injection side. By sealing the opening(s) in one or both of the cell-injection side and the specimen-injection side, no movement of the liquid level arises in the wells constituting a connecting tube via the channel and, in its turn, no transportation of the liquid arises in the channel. That is to say, it is possible to prevent cells from unexpected migration in the channel or a change in the concentration gradient of the specimen formed in the channel even though the apparatus is vibrated. By providing the means of transporting cells by injecting or aspirating/discharging a liquid, the cells can be easily aligned along the start line at one end of

the channel.

【0017】

Next, this structure will be illustrated by referring the model views Figs. 1(1) and (2). A raised bank 2 is formed on a substrate 1 and a channel 9 having resistance to the passage of cells is formed between the bank 2 and a glass substrate 10. First, a cell suspension is supplied by a liquid-injection means (a pulse pump 7 in Fig. 1) from a cell-injection port 5 into a cell-holding well 3 via an injection pipe 8. The cells are brought together at one end of the channel 9 having resistance to the passage of cells due to the flow of the liquid and the excessive liquid is discharged from a specimen-injection port 6 (see 12 in (2)). Since a cell transported to the end of the channel 9 blocks the liquid flow, the liquid flow passes through a cell-free part. As a result, the space is filled up with other cells and thus cells are aligned at the end of the channel 9. Although it is not necessary to strictly define the injection speed of the cell suspension, it is favorable to control the transportation speed to about 30 to 40 $\mu\text{m}/\text{sec}$ in the case of, for example, using neutrophils or eosinophils and the channel gap size being 5 μm . Next, the liquid transportation is stopped by the pulse pump 7 and the injection pipe 8 is closed, thereby sealing the cell-injection port. Then a chemotactic factor is injected from a specimen-injection port 6. Since the cell-injection port is sealed in this step, the back-flow of

the liquid can be prevented and the alignment of the cells at one end of the channel 9 is not disordered. Also, no unexpected migration of the liquid arises in the channel. Thus, the cells perceive the concentration gradient of the specimen (for example, a chemotactic factor) having been stably formed in the channel 9, undergo deformation and thus migrate toward the specimen-holding well side via the channel 9. The passage is observed through the glass substrate 10 by using a detector 11.

【0018】

As an example of the pulse pump to be used as the liquid-injection means, an apparatus for pulsing liquid transportation in small portions through a liquid-transport pipe, which is driven by compressed air pressure, may be cited. By using this apparatus, a liquid can be quantitatively transported at an order of 1 μ l to 1/10 μ l. It is also possible to seal the transport pipe. As such an apparatus, for example, there has been known MSL Active Microfluidic Chip Control Hardware (trade name) marketed from Fluidigm Corporation (South San Francisco, CA). In addition to the above-mentioned one, there has been known an apparatus with the use of the vibration of a piezoelectric element as a means of pulsing liquid transportation. Use can be made of any of these apparatuses as the liquid-injection means in the present invention. Since a pipe cannot be sealed in the apparatus with the use of the vibration of a piezoelectric element, it is necessary to separately provide a sealing means

in the case of using it.

【0019】

As the liquid-injection means, it is also possible to employ various means other than a pulse pump. For example, use can be made of a syringe represented by 13 in Fig. 2. By using this syringe which is driven by a stepping motor (also called a pulse motor), a liquid can be quantitatively transported. It appears favorable to use this syringe, since the injection port 5 is self-sealed by stopping the liquid transportation without causing back-flow of the liquid.

【0020】

It is also possible to seal the injection port by using a valve as shown in, for example, Figs. 3(1) and (2). Fig. 3(1) shows a case wherein a valve 16 is provided in an injection pipe 8, while (2) shows a case wherein a valve 16 is provided between a cell suspension tank 15 and an injection pipe 8. In Fig. 3, 14 stands for a liquid-injection means such as a pulse pump or a syringe. The valve 16 may be substituted by another member having a function comparable to a valve. For example, the liquid flow can be stopped by deforming a pipe made of a flexible and elastic material under pressure.

【0021】

The cell-injection port or the specimen-injection port formed on the substrate can be sealed by various means. For example, use can be made of a slide-type switching member represented

by 17 in Fig. 4. Fig. 4(1) shows a case wherein a cell-injection port 5 is open for injecting cells. After injecting the cells from the cell-injection port 5, the cell-injection port 5 is closed by sliding the slide-type switching member 17 as shown in (2). Next, the thus injected cells migrate on the flow of a liquid (for example, a buffer solution), which is supplied by a liquid-injection means 14 and transported through an injection pipe 8, to the end of a channel 9. After the migration of the cells, the pipe 8 is sealed with the use of a means appropriately selected from the above-described ones. The slide-type switching member can be easily switched with the use of, for example, a stepping motor with controllable rotation speed.

【0022】

Fig. 5 shows a modification of the structure shown in Fig. 4. Fig. 5(1) shows a case wherein a specimen-injection port 6 is closed when a cell-injection port 5 is opened, while (2) shows another case wherein a specimen-injection port 6 is opened when a cell-injection port 5 is closed.

【0023】

Fig. 6 shows a case wherein a cell-injection port 5 is sealed with a flexible stopper 19. Namely, the cell-injection port 5 is tightly sealed with the stopper made of, for example, a filmy silicone rubber, polyurethane, polyethylene, crude rubber or the like having a high elasticity (Fig. 6(1)). Cells

are injected by using a cell injector 20 penetrating through the stopper 19 (Fig. 6(2)). After injecting the cells, the injector 20 is drawn out. Thus, the hole in the stopper 19 is filled up owing to its elasticity and the cells 12 are brought together at an end of the channel 9 by the transported liquid flow (Fig. 6(3)). As a substitute for the stopper, it is also possible to employ a tap or the like which is lightly closed in usual but easily allows the penetration of the injector.

【0024】

As a substitute for the structures of Figs. 1 to 6, moreover, use can be also made of a structure shown in, for example, Fig. 7 wherein a liquid is aspirated and discharged from the side of a specimen-holding well 4, which is located in the opposite side to a cell-holding well 3 having a bank 2 between them, and thus cells 12 are brought together at one end of a channel 9 of a cell-holding well 3. Although the liquid is aspirated with a syringe 13 in Fig. 7, it may be substituted by another means having a similar function such as a pulse pump.

【0025】

The apparatus according to the present invention may have a structure in which a liquid (a medium of the cell suspension) is circulated. Figs.8(1) to (4) present model views of such an apparatus. Fig.8(1) shows a case wherein a cell-holding well 3 has an injection pipe 8 while a sample-holding well 4 has an aspiration discharge pipe 21 and a specimen-injection port is

sealed with a flexible stopper 19. As Fig. 8(4) shows, the liquid is circulated by using a means of transporting the liquid in a single direction, for example, a pulse pump 7. Figs. 8(1) and (2) show each a case wherein cells are injected from the cell-injection port 5, while Figs. 8(3) and (4) show each a case wherein the liquid is transported in the direction indicated by an arrow so as to bring the cells together at one end of a channel 9. In this case, a chemotactic factor is injected from the specimen-injection port 6 through the stopper 19. The specimen-injection port 6 may be sealed with the use of a means other than the stopper, for example, a slide-type switching member, a valve, a tap or the like.

【0026】

Fig. 9 shows an example, which is a substitute for the structure of Fig. 8, wherein a cell-injection port 5 is sealed. As Fig. 9 shows, the cell-injection port 5 can be sealed with a flexible stopper 19. Alternatively, the sealing may be made with the use of a slide-type switching member, a valve, a tap or the like.

【0027】

Fig. 10 shows another modification of the apparatus according to the present invention wherein a cell-injection port 5 and a specimen-injection port 6 are both sealed. In the case of Fig. 10, the injection ports 5 and 6 are sealed respectively with flexible stoppers 19 and cells and a factor are injected through the respective stoppers. To bring together the cells

at one end of a channel 9, liquid-transport means provided with a member (for example, a syringe 13) of stopping the migration of the liquid after the liquid transportation are provided in both of the cell-holding well 3 side and the specimen-holding well 4 side. By driving these means in conjunction, a liquid is transported from the cell-holding well 3 side toward the specimen-holding well 4 side. It is needless to say that another means of sealing the injection ports such as a slide-type switching member or the like may be used as a substitute for the stopper.

【0028】

Moreover, the present invention includes in its scope an integration apparatus for detecting chemotaxis of cells consisting of a plural number of units with the use of the above-described apparatus for detecting chemotaxis of cells as a single unit. For example, Fig. 11 shows a model assembly wherein units each having a sealed cell-injection port are connected via an injection pipe 8 so as to bring together the cells in individual cell-holding wells at the end of a bank at the same time. In the case of Fig. 11, it is favorable that the injection pipe 8 is sealed at individual units with, for example, valves 16 so as to ensure the sealing in the cell-injection port 5 side. The means for sealing the specimen-injection port and the pipe may be appropriately selected from among various members as cited above.

【0029】

Fig. 12 shows a model view of an integration apparatus having the units of the type shown in Fig. 10. Stoppers 19 in this figure may be substituted by other means. By using this apparatus, effects of various specimens on a single type of cells can be examined simultaneously. Alternatively, a cell-injection port 5 and specimen-injection ports 6 may be interchanged each other. Owing to this structure, reactions of a single specimen with various type of cells can be examined simultaneously.

【0030】

Moreover, the present invention includes an integration apparatus consisting of a plural number of integration units and an integration apparatus consisting of integration units of multiplicity of types.

【0031】

According to the present invention, such an apparatus can be downsized as a whole and a sample can be treated in a microquantity. By integrating a plural number of units, furthermore, a large number of specimens can be treated simultaneously. In addition, a liquid-aspiration/injection program can be easily controlled in the apparatus according to the present invention, which makes it suitable for fabricating an automated apparatus.

【0032】

Next, each part of the apparatus according to the present invention will be illustrated by reference to specific examples. However, it is to be understood that these examples are intended to illustrate the present invention, not by way of limitation, and variations can be made without departing from the spirit and scope of the invention.

【0033】

1) Structure of unit

As Fig. 1 and other figures show, it is preferred that a bank 2 and wells 3 and 4 are integrally formed on a substrate 1. An optically flat glass substrate 10 is mechanically pressed against the bottom face of the substrate 1. The substrate 1 and the glass 10 may be bonded together by heating.

【0034】

2) Well

The wells 3 and 4 aim at respectively holding a cell suspension and a specimen such as a chemotactic factor-containing solution or an inhibitor-containing solution. The capacity of the wells is not particularly restricted, so long as a liquid can be held therein in the minimum amount needed. For example, it is sufficient that the depth ranges from about 0.05 to about 0.1 mm, the width and the length are each about 1.2 mm.

【0035】

3) Channel

Next, an example of the structure of a channel 9 (see Fig. 1)

will be illustrated by referring to Fig. 13. The channel 9 is a space provided between a bank 2 (a convex on a substrate 1) partitioning the wells 3 and 4 at both ends and the glass substrate 10. A flat terrace 23 is provided on the bottom face of the bank. Although the bank 2 is not restricted in size, it is preferred, for example, that the height of the bank 2 (i.e., the distance between the glass substrate 10 and the terrace 23) ranges from about 0.003 to about 0.03 mm, while the length in the direction toward the opposite well ranges from about 0.1 to about 0.5 mm and the length in the direction orthogonal to the direction toward the opposite well is about 1.2 mm. Needless to say, these dimensional factors may be varied depending on the purpose such as the type of the subject cells.

【0036】

The distance between the terrace 23 and the glass substrate 10 may be appropriately controlled depending on the cells to be treated. Usually, it ranges from 3 to 30 μm . That is to say, the distance may range from 3 to 8 μm (for example, 4, 5 or 8 μm) in the case of treating neutrophils, eosinophils, basophils, monocytes/macrophages, T cells, B cells and the like, and from 6 to 20 μm in the case of treating cancer cells and cells existing in tissues.

【0037】

It is also possible to form a multistage terrace 23 to facilitate the migration of the cells toward an end of the channel 9.

【0038】

In a preferred embodiment, a plural number of barriers 24 are formed on the bottom face (the terrace 23) of the bank 2 to provide grooves 25 through which cells pass, as shown in Figs. 14(1) and (2). Fig. 14(1) is a sectional view of the bank 2 having the barriers 24, while (2) is a top plan view showing the terrace 23, the barriers 24 and the grooves 25.

【0039】

In case where barriers 24 are formed on the terrace 23, the grooves 25 provided by the barriers 24 may have an arbitrary cross-sectional shape, for example, a V-shaped section, a convex section or a semicircular section. The grooves 25 have a width and a depth fit for the diameter or deformability of cells. Fig. 14(3) is a sectional view showing a case wherein the grooves 25 have a V-shaped section.

【0040】

The width of a groove 25 usually may range from 3 to 50 μm . That is, an appropriate width may be selected depending on the cell type. The width may range from 3 to 20 μm (for example, 4, 8 or 10 μm) in the case of treating neutrophils, eosinophils, basophils, monocytes/macrophages, T cells, B cells and the like, and from 8 to 20 μm in the case of treating cancer cells and cells existing in tissues. The number of the grooves 25 is determined depending on the width of the barriers 24 and the width of the grooves 25 concerning the width of the channel 9.

In case where the width of the channel 9 is 1 mm, the width of the barriers 24 is 10 μ m and the width of the grooves 25 is 5 μ m, for example, the number of grooves is 66 at the largest.

【0041】

It is also possible to form arrays of barriers 24 in two positions in both sides of the terrace 23 which is formed on the bank 2 (see Figs. 15(1) and (2)). By using this structure, cells having passed through the grooves can be easily observed and counted. By providing a mark 26 at an appropriate position in the center terrace 23, positioning can be easily made under a camera or a microscope (26 in Fig. 15). It is desirable that the terrace located at the center has an area which can be included in the microscopic field. Fig. 15(1) is a top plan view while (2) is a sectional view.

【0042】

4) Construction of well and channel

For the substrate 1, it is preferable to use a material which can be easily fine processed and is relatively inert to cells, for example, single-crystal silicon. The barriers 24 and the grooves 25 can be easily constructed by subjecting the single-crystal silicon to photolithography or etching (for example, wet etching or dry etching) employed in manufacturing integrated circuits. The wells 3 and 4, which are relatively larger than the barriers 24 and the grooves 25, can be constructed by using various known engineering techniques such

as sand blasting and dry etching.

【0043】

In addition to single-crystal silicon, use can be made of hard glasses, hard plastics, metals, etc., so long as a microstructure can be constructed in the channel. Polydimethylsiloxane (PDMS) may be cited as an example of the plastics suitable for the construction of a microstructure. In the case of using plastics, it is preferable to employ a treatment for making the surface hydrophilic, for example, forming a hydrophilic film on the surface. To facilitate the observation of the cells, it is also preferable to subject the surface at least having the terrace 23 to specular finishing by, for example, silver deposition. It is also possible to separately construct the bank 2 and the wells 3 and 4 and then combine them together.

【0044】

5) Glass substrate

As shown in Fig. 1 and other figures, the glass substrate 10 is tightly pressed against the substrate 1 to provide a space in which a liquid is held, thereby enabling the observation of cells passing through the channels. Thus, the glass substrate 10 should remain optically transparent and flat and provide a plane to which cells can adhere. Use can be made therefor of glass as well as plastics such as transparent acrylic resins, so long as the above objects can be achieved thereby. Although

its thickness is not particularly restricted so long as no strain arises in the step of pressing against the substrate, the thickness adequately ranges from 0.1 to 2 mm. In the case where cellular constituents are fluorescent labeled and observed, a thinner glass substrate 10 is preferred.

【0045】

In the case where the substrate 1 is made of a silicone wafer, it can be integrated together with the glass substrate 10 by mechanically pressing. Alternatively, they may be bonded together by heating to 200 to 400°C. In this case, however, it is needed to select materials for the substrate 1 and the glass substrate 10 so that the coefficients of thermal expansion and the coefficients of thermal shrinkage thereof agree with each other.

【0046】

6) Pipe

It is generally preferred that the injection pipe 8 and the aspiration discharge pipe 21 are made of flexible materials. In the case of using a pulse pump 7, it is particularly needed that these pipes follow-up minor movements. Use can be made of, for example, PDMS, polyethylene, vinyl chloride, etc. therefore.

【0047】

7) Arrangement of a plural number of units

By referring two wells connected to each other via a channel

as a single unit, a plural number of units may be arranged and integrated on a single substrate. Thus, an apparatus whereby a large number of specimens can be simultaneously treated can be obtained. Units of the same type may be arranged in parallel or units of different types may be arranged. Namely, arbitrary arrangement may be employed depending on the purpose. In the case where a unit having two wells connected to each other via a channel has a major side length of 2.9 mm and a minor side length of 1.2 mm, for example, 14 (i.e., 7 in column x 4 in row) can be provided at intervals of 0.8 mm on a rectangular substrate of 16 mm in width and 10 mm in length.

【0048】

Such assemblies consisting of a plural number of units as described above may be further integrated. It is also possible to integrate different types of units together.

【0049】

In the case of integrating a plural number of units, use may be made of one glass substrate 10 covering all of the units.

【0050】

8) Detection means

The detection means to be used in the present invention may be any means so long as cells which are passing through the channel 9 or have migrated therethrough can be detected thereby. If necessary, it involves a means of recording the detection data. Any means known as a means of detecting and recording cells is

usable therefor. Use can be made of, for example, a microscope optionally combined with a video camera. It is also possible to employ a system having an objective lens provided with a CCD camera. For the detection in integrated units, it is preferable to employ a system wherein the channels of the units are successively scanned along with an objective lens.

【0051】

As shown in Fig. 1 etc., the detection means is usually provided below the channel 9 in a unit. In an automated apparatus having a plural number of units integrated together, it is also possible to employ a system wherein arrays of the units successively come to a detection part located at a definite position for detection and recording. In this case, the channels of the aligned units are scanned with the detector. Either one or more scanning detectors 11 may be employed. Owing to this constitution, a relatively small number of detectors suffice for the detection in a plural number of integrated units.

【0052】

Cells which are passing or have passed through the channel 9 can be detected and counted by directly observing the cells with a microscope. Alternatively, the detection and counting can be easily performed by preliminarily labeling the cells with a luminous or fluorescent substance and then capturing the luminescence or fluorescence in a conventional manner.

【0053】

9) Automatic controlling system

The apparatus according to the present invention can be easily controlled automatically. For example, use can be made of an autopipette whereby injection, transportation and discharge of cells or specimens such as a factor can be controlled with a computer, a pulse pump or a syringe driven by a stepping motor as a means of transporting a liquid, and a slide-type switching member for opening and closing an injection port. Thus, the operation order and the operation level of each member can be controlled by computerized programming. In the case of using a stopper as a substitute for the slide-type switching member for opening and closing an injection port, it is unnecessary to control the switching operation.

【0054】

In an integrated apparatus, it is preferable to employ a pipette having a multichannel syringe.

【0055】

【Effect of the Invention】

According to the structure of the present invention, it is possible to control the positioning of cells injected into a channel and bring together and align the cells at an end of the channel. It is also possible thereby to hold the cells in the above-described state and maintain a stable concentration gradient due to the diffusion of the specimen such as a

chemotactic factor in a channel. Accordingly, quantitative data certainly reflecting the effect of a chemotactic factor or an inhibitor and the properties of cells can be obtained.

【0056】

By employing the structure according to the present invention, it is also possible to prevent disorders in the cell line and in the concentration gradient of a specimen formed in the channel even though the apparatus is unexpectedly vibrated. Thus, the movements of the cells can be exactly understood.

【0057】

By using the structure according to the present invention, furthermore, the apparatus can be downsized. When this apparatus is applied to an apparatus for detecting chemotaxis of cells or separating chemotactic cells, namely, samples can be used in an amount 1/500 to 1/1000 times as much in the conventional cases with the use of a Boyden chamber. That is to say, a biological sample such as whole blood per se can be used as a sample in the apparatus according to the present invention. In the case of using whole blood as a sample, for example, measurement can be made by using 0.1 μ l or less of the blood in the case of detecting the chemotaxis of neutrophils and about 1 μ l of the blood in the case of detecting eosinophils, monocytes or basophils.

【0058】

The structure according to the present invention achieves a

remarkable technical merit that the positioning of cells in a well can be delicately controlled and thus the apparatus can be easily automated.

【0059】

The unit of the apparatus according to the present invention can be in a microsize and thus a plural number of the units can be integrated together, which brings about another merit that an apparatus whereby a large number of samples can be simultaneously treated can be fabricated. In this case, an apparatus having an automated system of injecting and detecting liquids can be easily fabricated.

【0060】

In integrating a plural number of units, detection and separation for different purposes can be simultaneously carried out by combining and integrating units of different types together. Thus, the treatment efficiency can be elevated. In the case of an apparatus for detecting chemotaxis of cells, for example, the detection of various chemotactic factors or inhibitors for a single type of cells or the detection of the chemotaxis of different types of cells for a single chemotactic factor can be carried out at once.

【Brief Description of Drawings】

【Fig. 1】 is a model view showing an example of an apparatus for detecting chemotaxis of cells in which cells are brought together at one end of a bank through the transportation of a

liquid from the cell-injection port side. In this figure, an arrow indicates the transportation direction of the liquid filling up the apparatus.

【Fig. 2】 is a model view showing a case wherein a syringe is employed as a substitute for the pulse pump shown in Fig. 1.

【Fig. 3】 is a model view showing a case of using a valve as a sealing means. In this figure, an arrow indicates the transportation direction of the liquid filling up the apparatus.

【Fig. 4】 is a model view showing a case of using a slide-type switching member as a sealing means.

【Fig. 5】 is a model view showing a case wherein a specimen-injection port is switched on/off in addition to the structure as shown in Fig. 4.

【Fig. 6】 is a model view showing a case of using a flexible stopper as a sealing means.

【Fig. 7】 is a model view showing an example of an apparatus for detecting chemotaxis of cells in which cells are brought together at one end of a bank through the aspiration and discharge of a liquid from the specimen-injection port side. In this figure, an arrow indicates the transportation direction of the liquid filling up the apparatus.

【Fig. 8】 is a model view showing a structure of the same type as in Fig. 7 wherein a liquid is circulated. In this figure,

an arrow indicates the transportation direction of the liquid filling up the apparatus.

【Fig. 9】 is a model view showing a structure wherein a cell-injection port is sealed in the type of Fig. 8. Figs. 9(1) and (3) are sectional views, while (2) and (4) are respectively top plan views. In this figure, an arrow indicates the transportation direction of the liquid filling up the apparatus.

【Fig. 10】 is a model view showing a structure wherein a cell-injection port and a specimen-injection port are both sealed.

【Fig. 11】 is a model view showing a case wherein a plural number of units of the type shown in Fig. 6 are integrated.

【Fig. 12】 is a model view showing a case wherein a plural number of units of the type shown in Fig.10 are integrated.

【Fig. 13】 is a sectional view showing an example of the structure of a bank and a channel.

【Fig. 14】 shows an example of a case wherein a barrier and a groove are formed in a channel.

【Fig. 15】 shows an example wherein arrays of the barriers constituting the grooves are formed at two positions on a terrace, wherein Fig. 15(1) is a top plan view while (2) is a sectional view.

【Description of Reference Numerals】

1: substrate

- 2: bank
- 3: cell-holding well
- 4: specimen-holding well
- 5: cell-injection port
- 6: specimen-injection port
- 7: pulse pump
- 8: injection pipe
- 9: channel having resistance to the passage of cell
- 10: glass substrate
- 11: detector
- 12: cell
- 13: syringe
- 14: liquid-injection means
- 15: cell suspension tank
- 16: valve
- 17: slide-type switching member
- 18: liquid-injection port
- 19: flexible stopper
- 20: cell injector
- 21: aspiration discharge pipe
- 22: specimen injector
- 23: terrace
- 24: barrier
- 25: groove in the direction toward the opposite well
across channel


26: mark for positioning on screen

【Name of Document】 DRAWINGS


【Fig.1】

- 1: substrate
- 2: bank
- 3: cell-holding well
- 4: specimen-holding well
- 5: cell-injection port
- 6: specimen-injection port
- 7: pulse pump
- 8: injection pipe
- 9: channel having resistance to the passage of cell
- 10: glass substrate
- 11: detector
- 12: cell

(1)

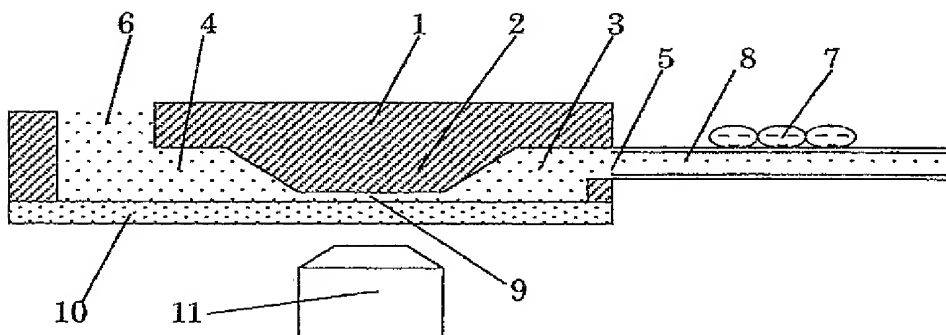


(2)

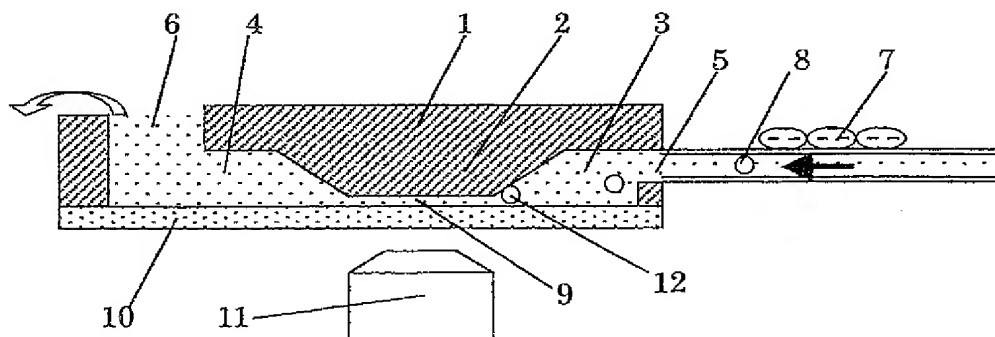

【Fig.2】


13: syringe

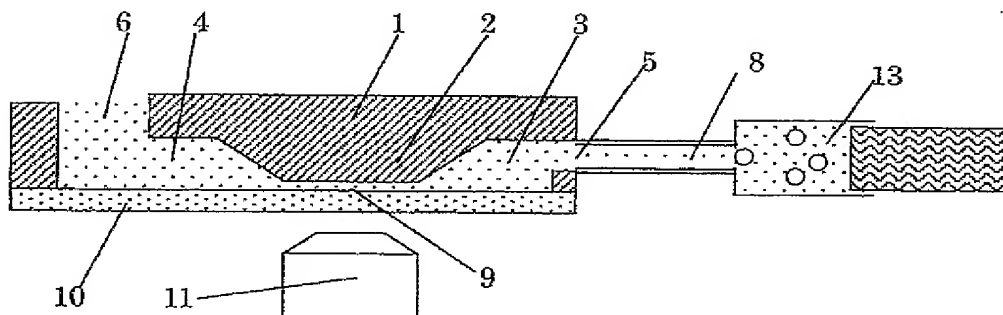


【Fig.3】

14: liquid-injection means
15: cell suspension tank
16: valve

(1)

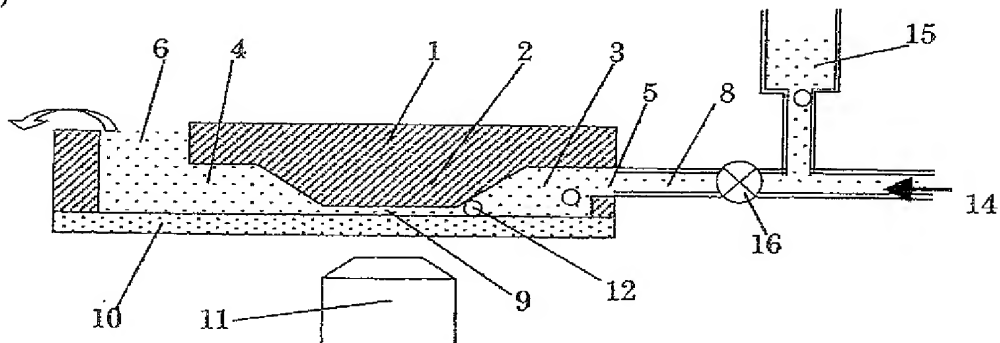


(2)

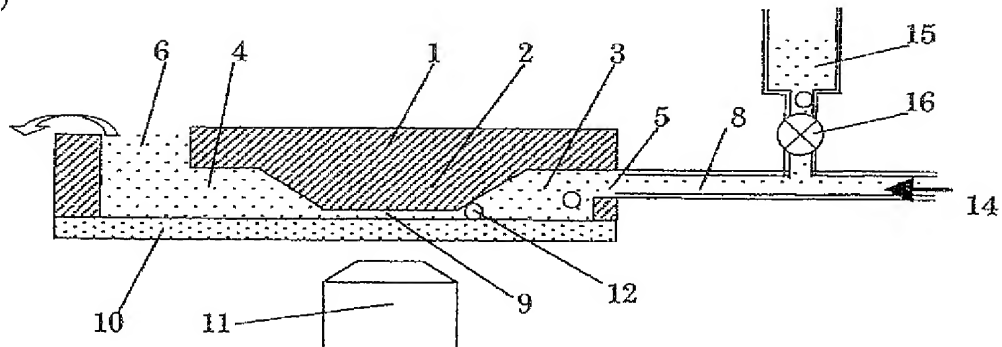


【Fig.4】

17: slide-type switching member
18: liquid-injection port

(1)

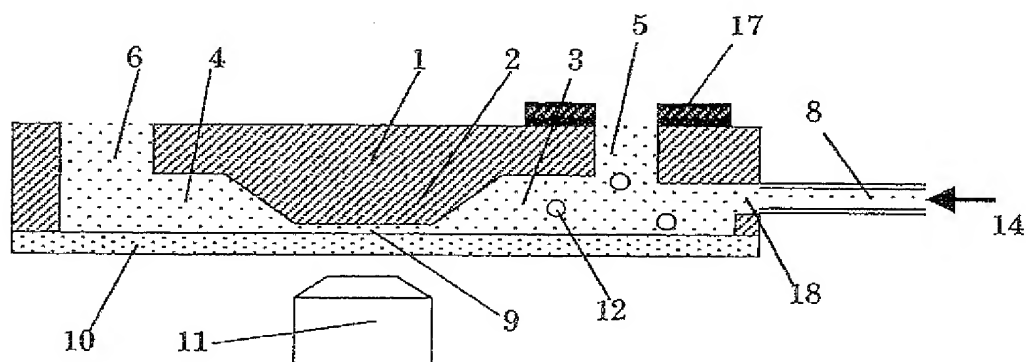


(2)

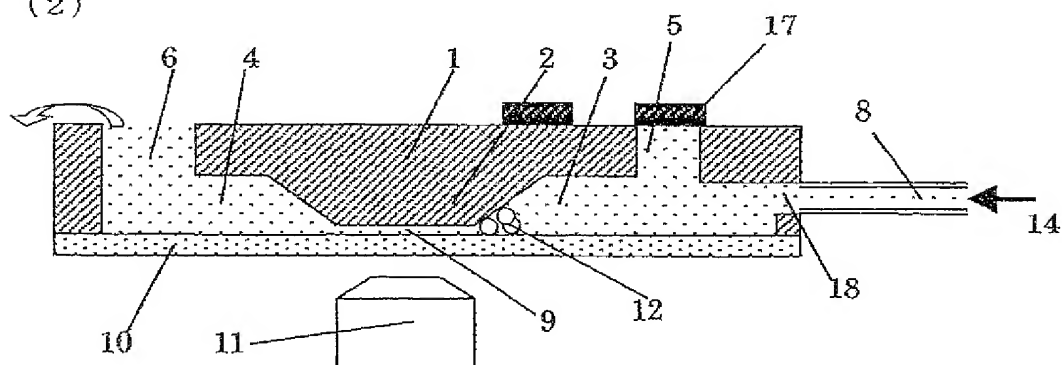


【Fig.5】

(1)

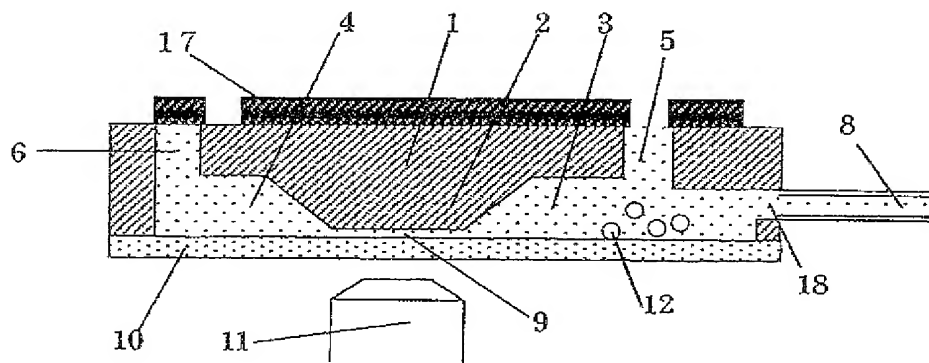


(2)

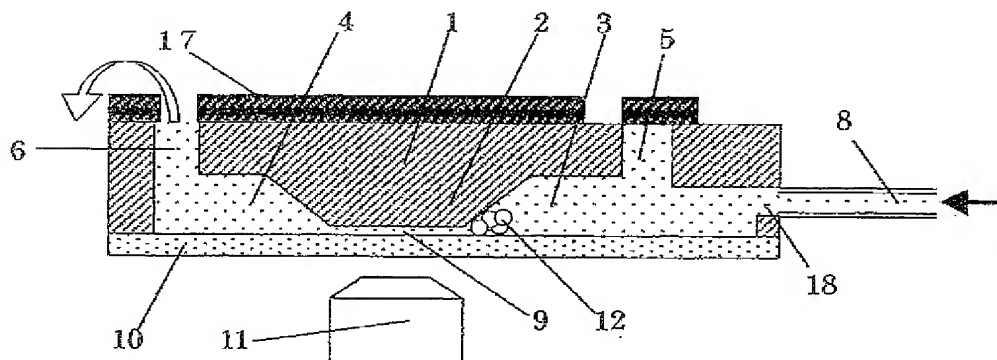


【Fig.6】

19: flexible stopper
20: cell injector

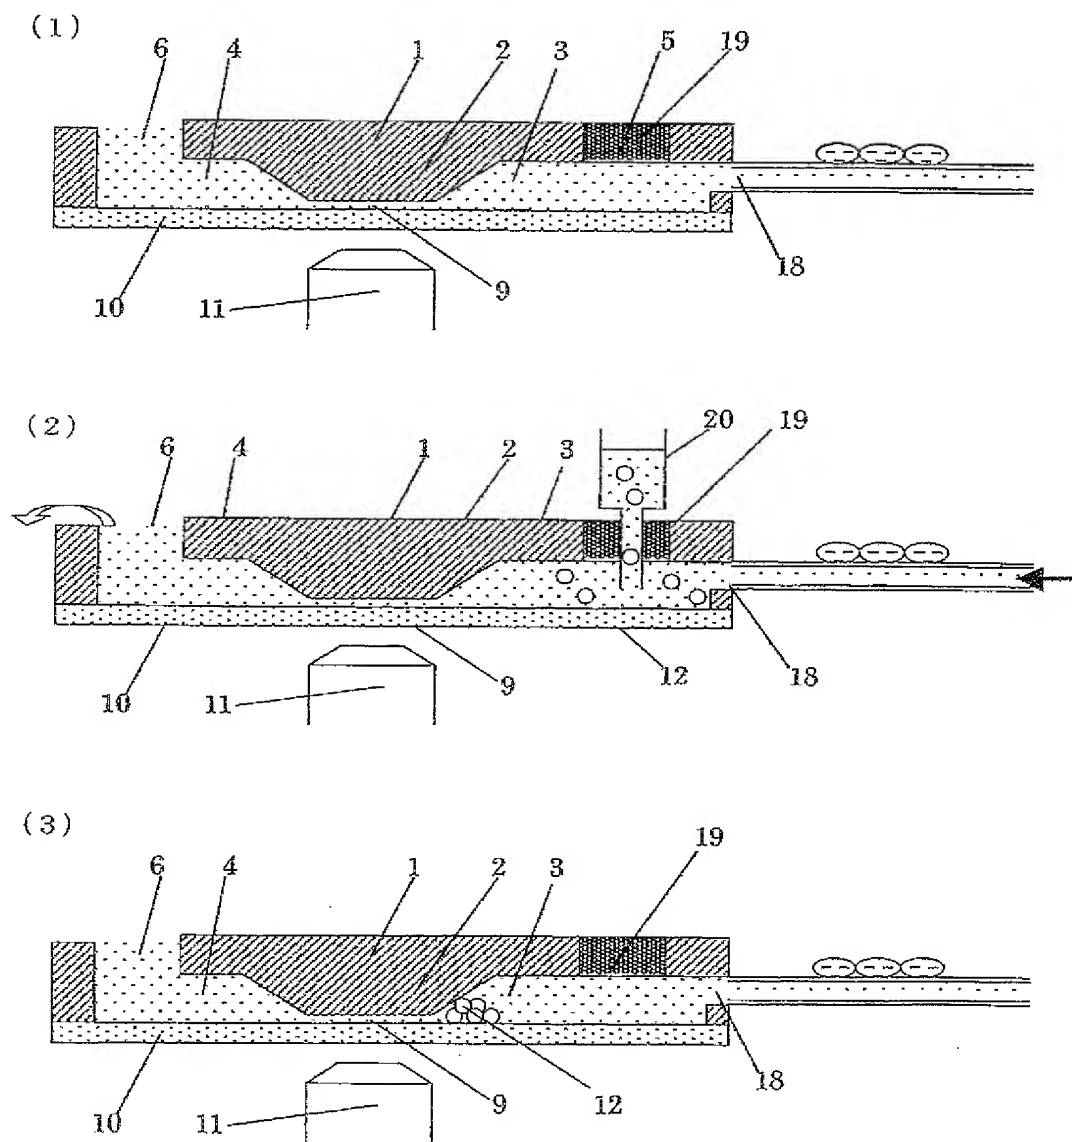


【Fig.7】


21: aspiration discharge pipe
22: specimen injector

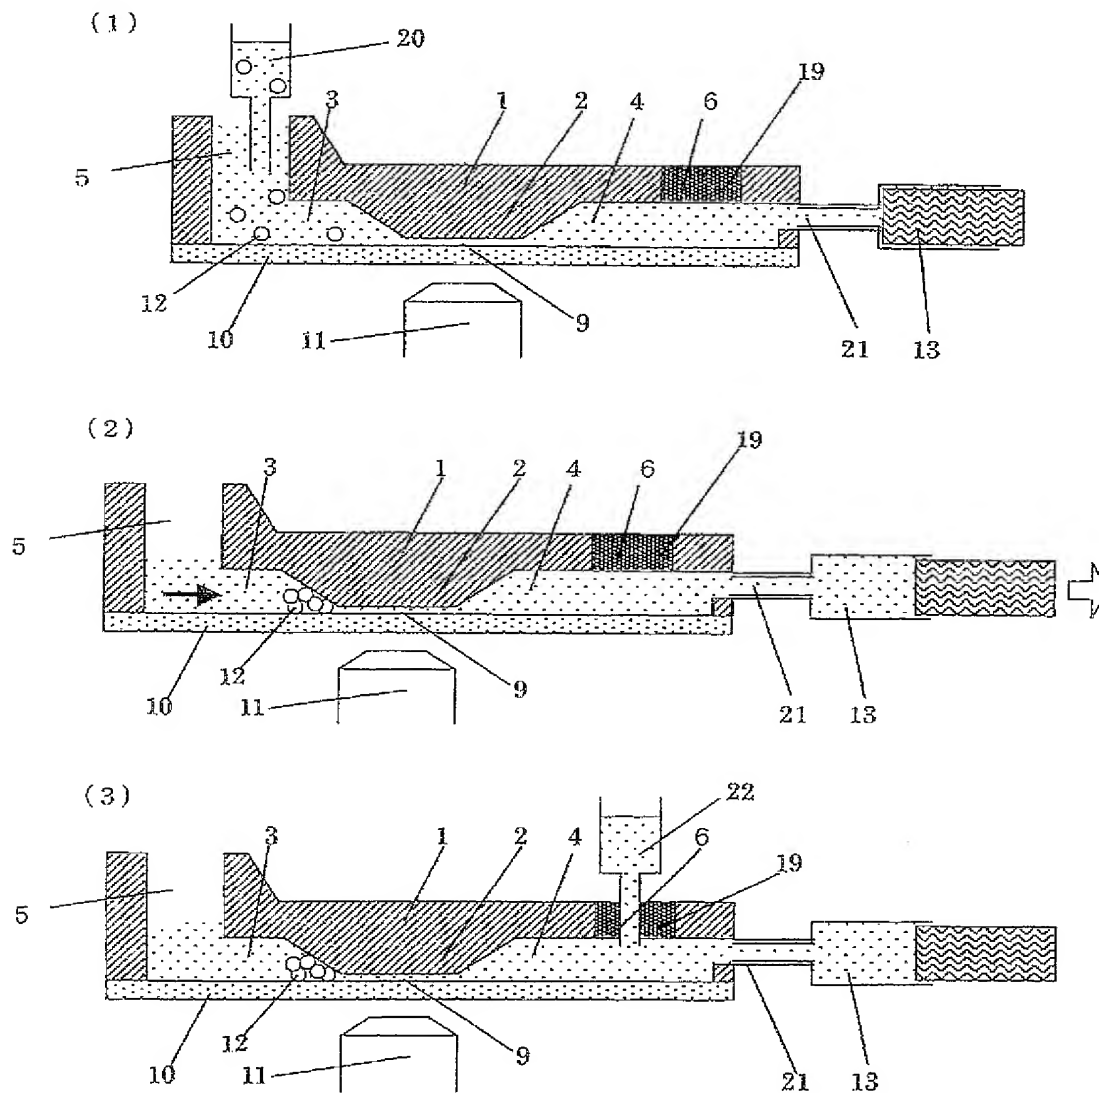


【Fig.8】

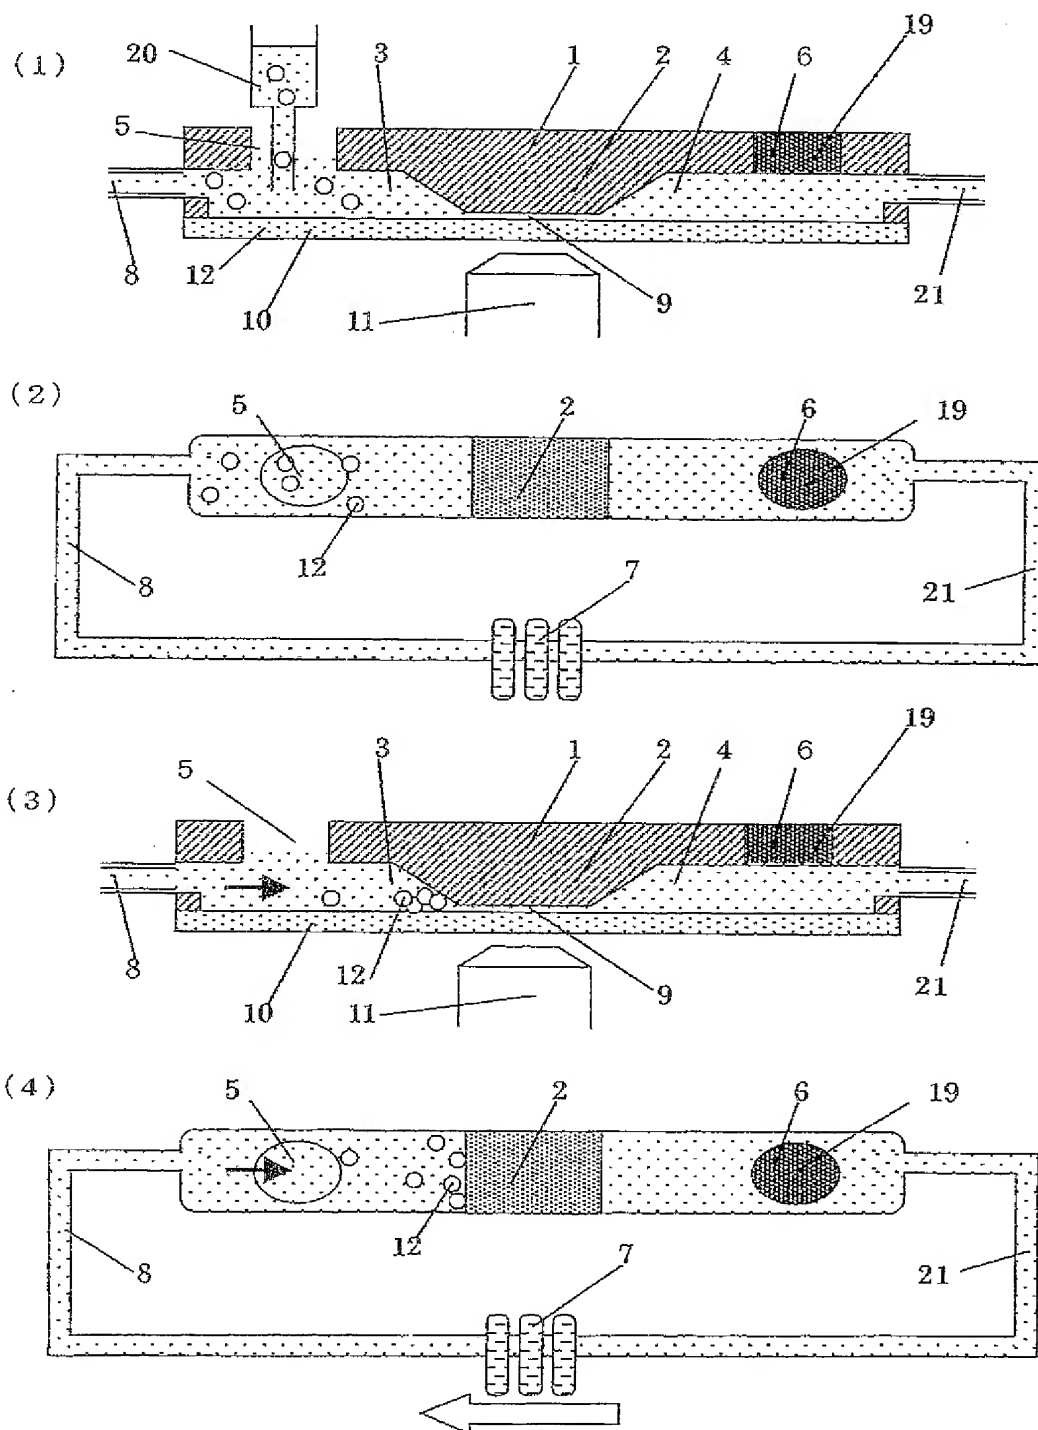


【Fig.10】

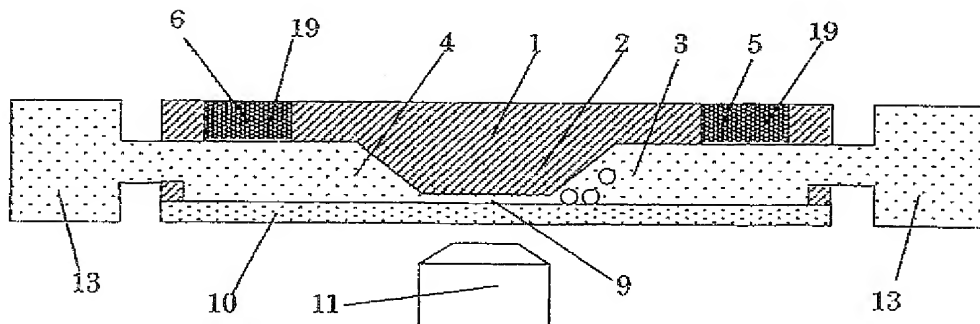

【Fig.11】

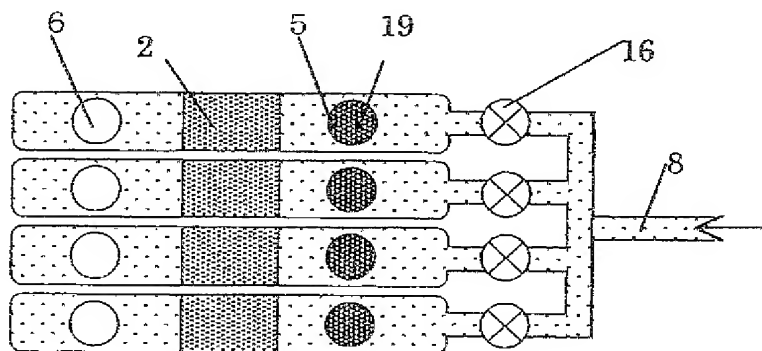


【Fig.12】

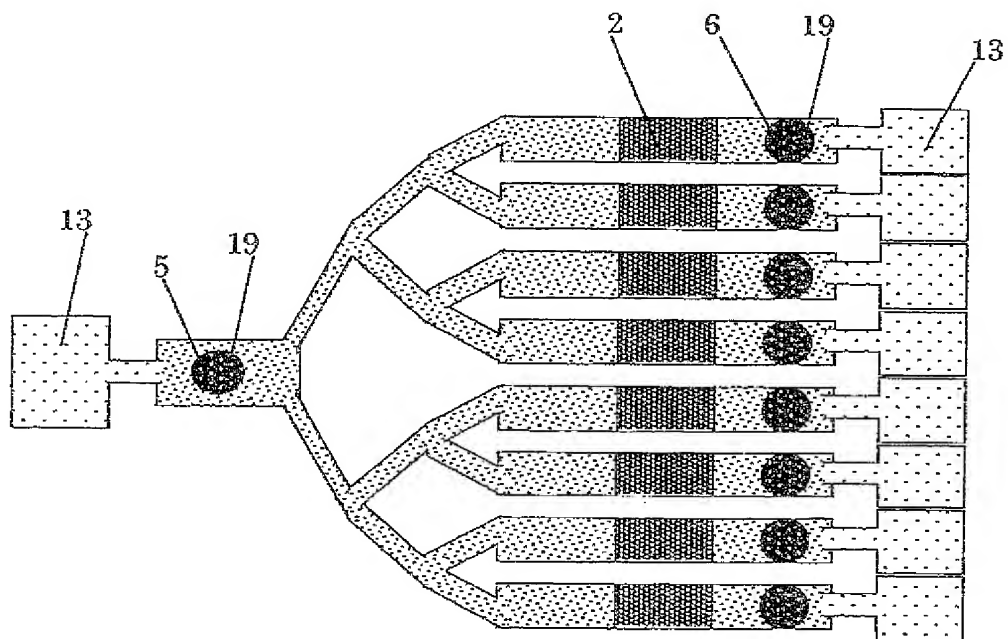

【Fig.13】

23: terrace

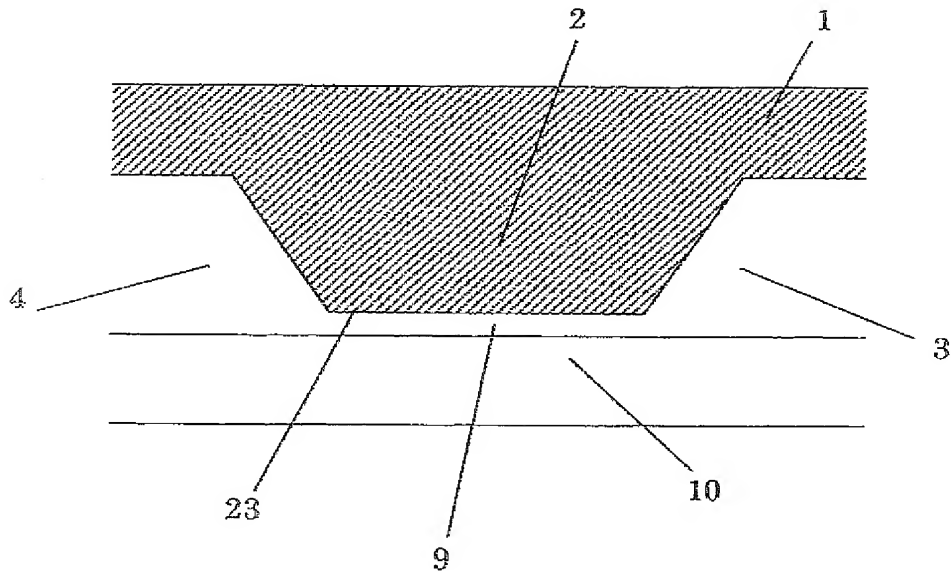


【Fig.14】


24: barrier

25: groove in the direction toward the opposite well
across channel


(1)

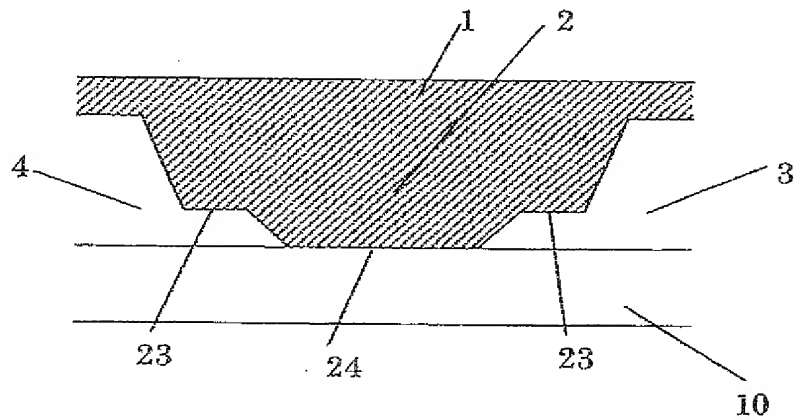

(2)

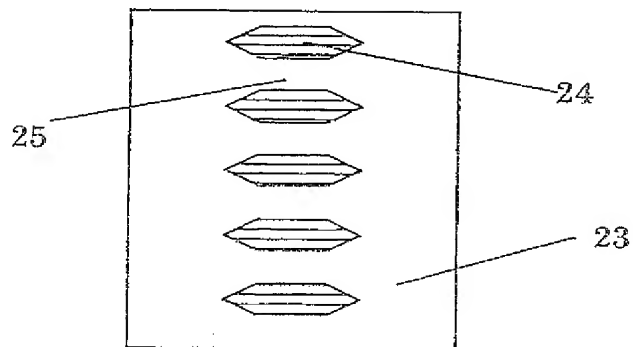


(3)

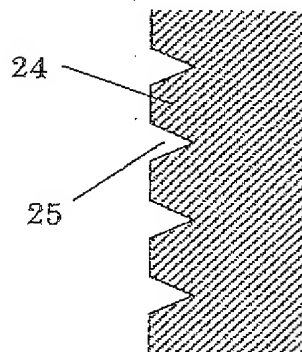

【Fig.15】

26: mark for positioning on screen

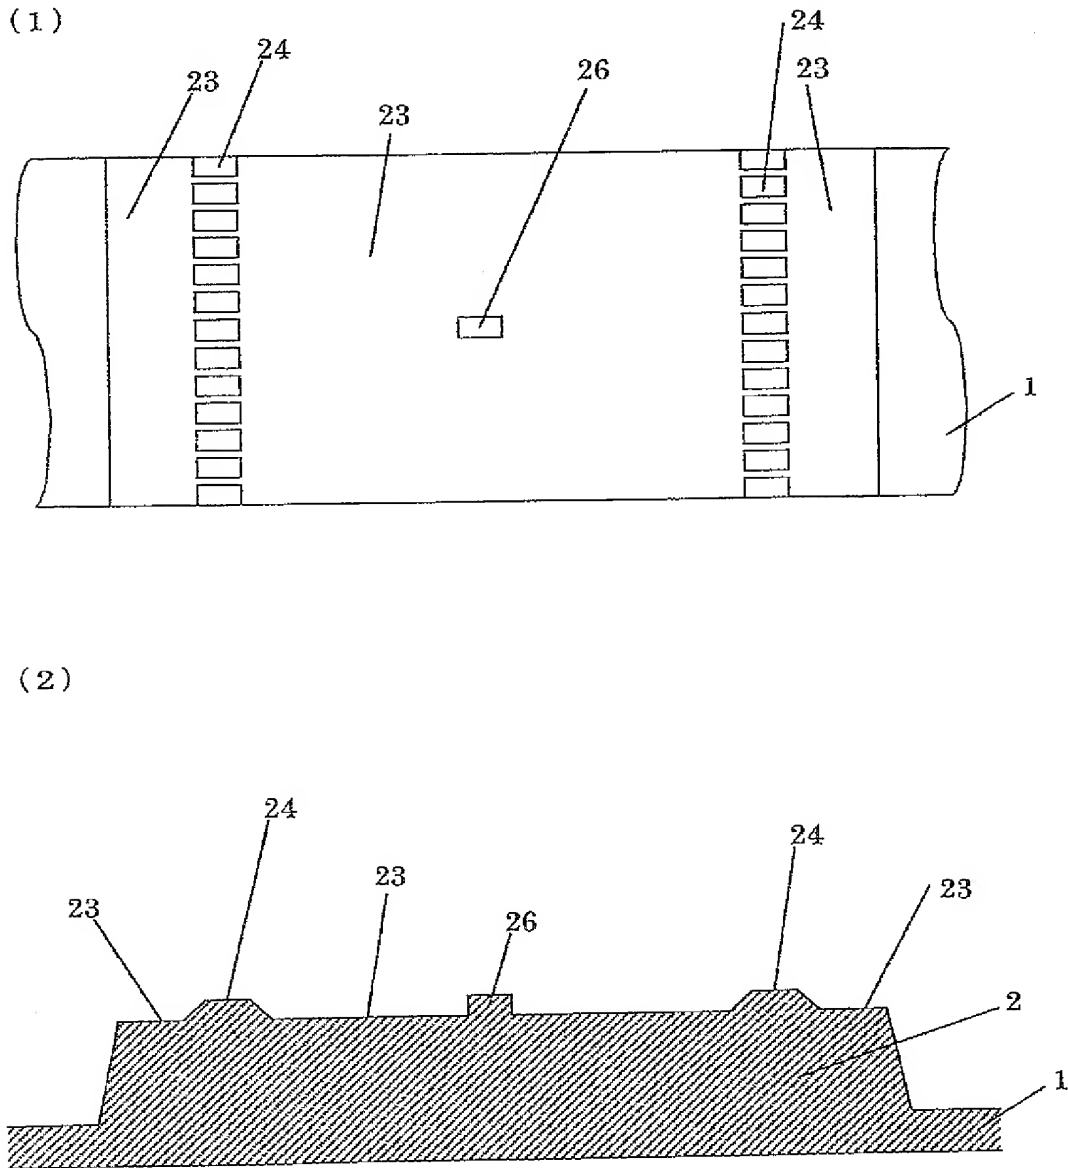

【Name of Document】 Abstract

【Abstract】

【Problem to be solved 】

The present invention relates to an improvement in an apparatus for detecting chemotaxis of cells. It aims at providing a structure for detecting chemotaxis of cells at an elevated accuracy with the use of a microquantity of cells. That is to say, an object of the present invention is to provide an apparatus for detecting chemotaxis of cells by which cell injection and position control can be easily carried out while ensuring the prevention of unexpected migration of the cells definitely positioned in a well or the injected sample so that a stable concentration gradient due to the diffusion of the specimen can be maintained and which ensures further automated operation and controlling.

【Means for solving problem】

The present invention relates to an apparatus for detecting chemotaxis of cells with a structure wherein plural wells are connected to each other via a channel and each well has an opening for injecting cells or a specimen, characterized by having a means of sealing the opening(s) in one or both of the cell-injection side and the specimen-injection side and said channel may have resistance to the passage of cells, moreover said

apparatus may have a means of transporting a liquid.

【Selected Figure】 Fig.1